



13a Process Flow Diagram

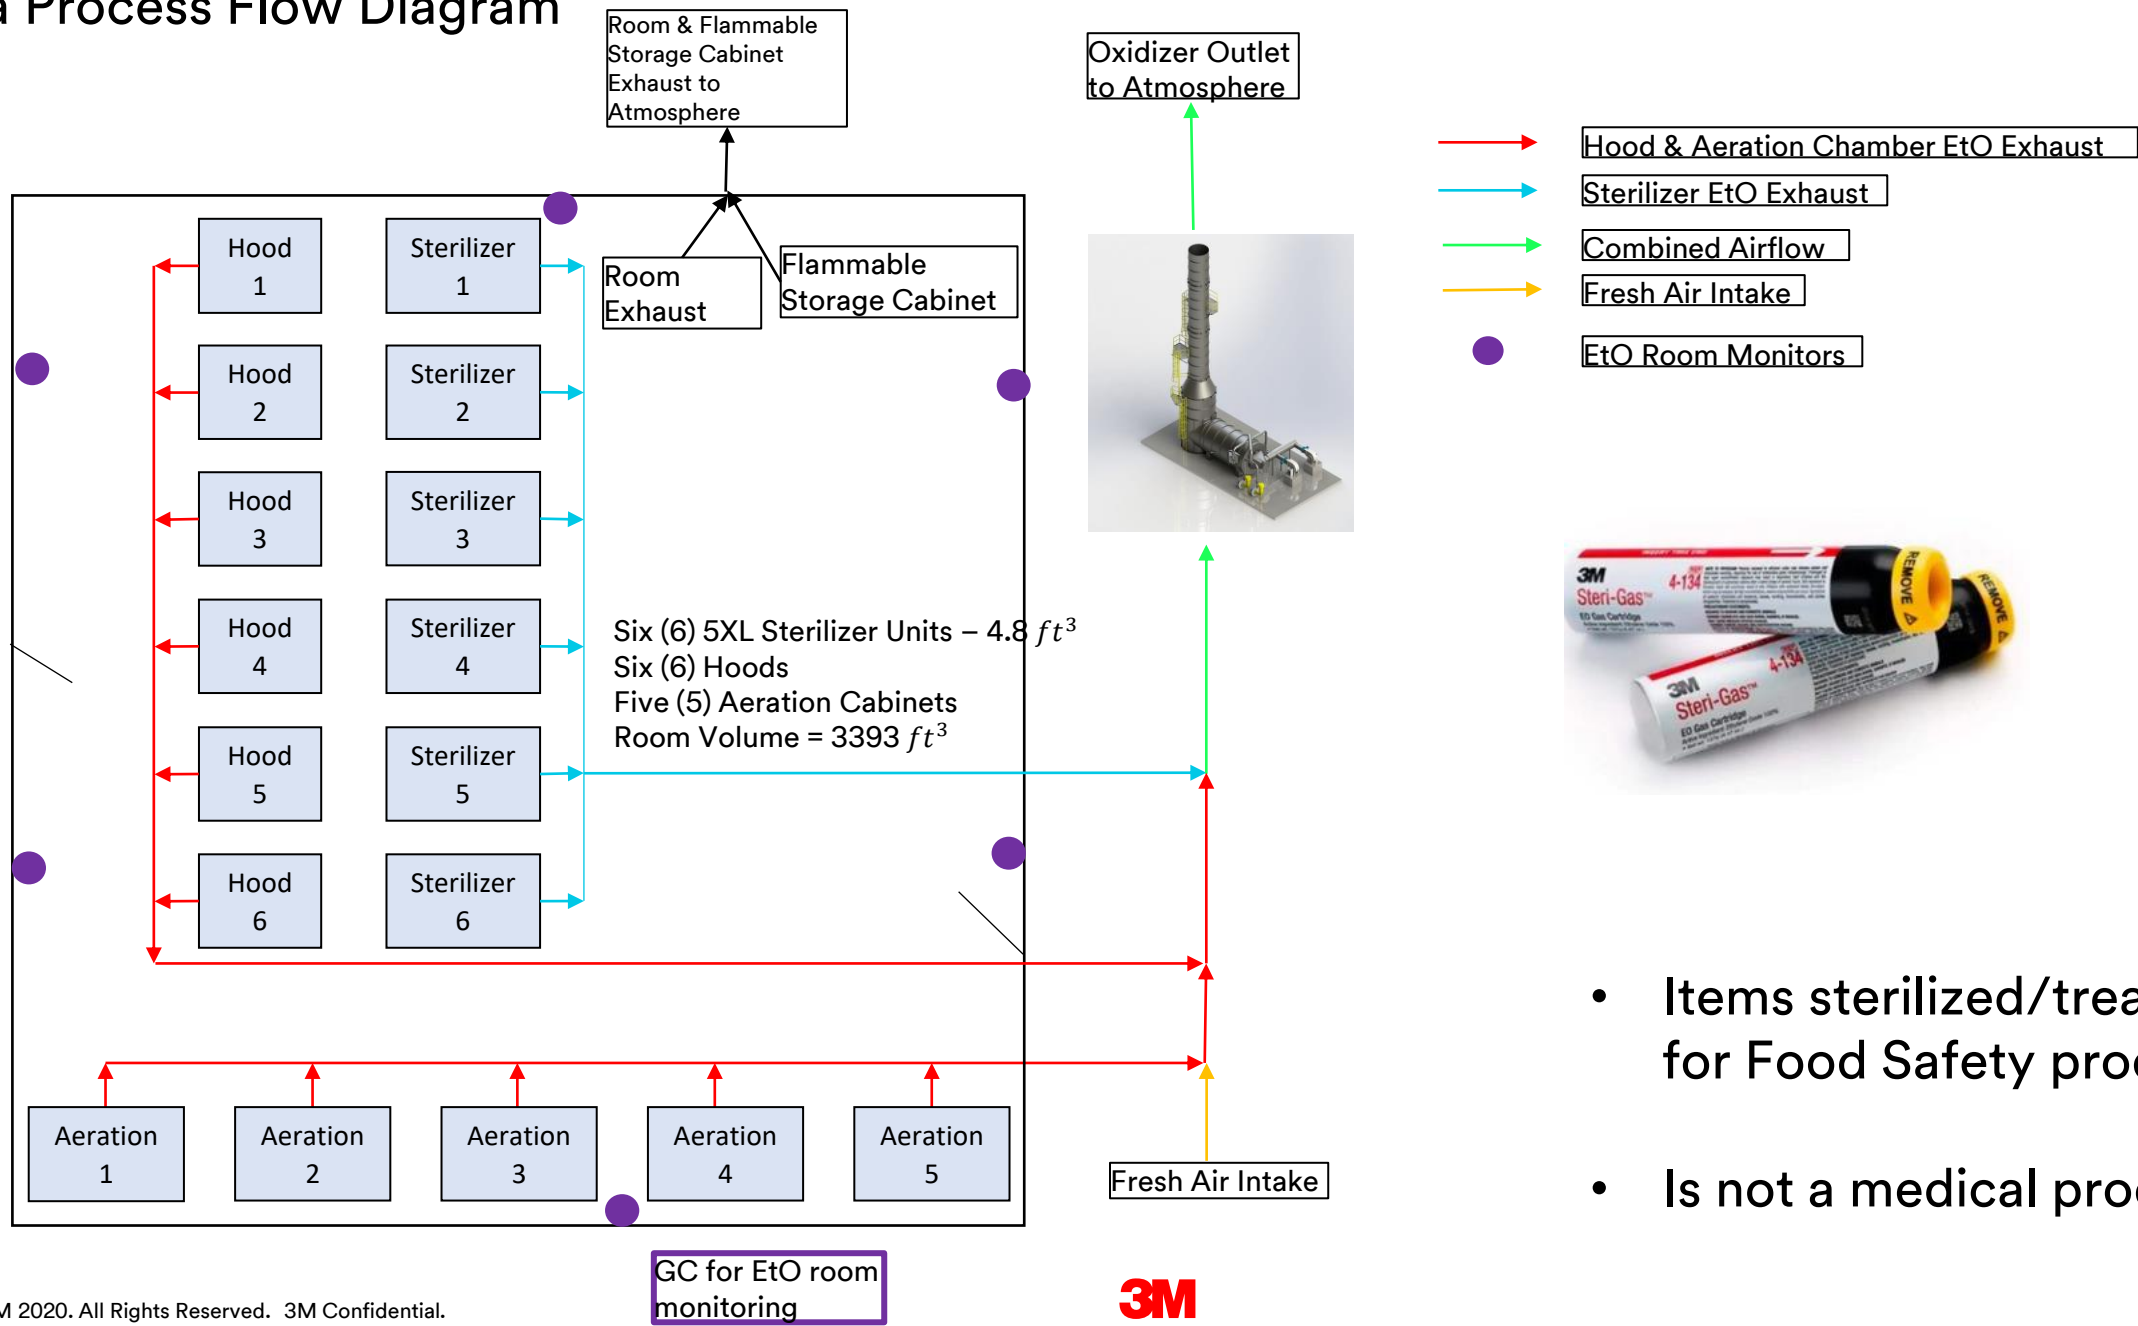

- Items sterilized/treated for Food Safety product
- Is not a medical product

13b Process Flow Diagram

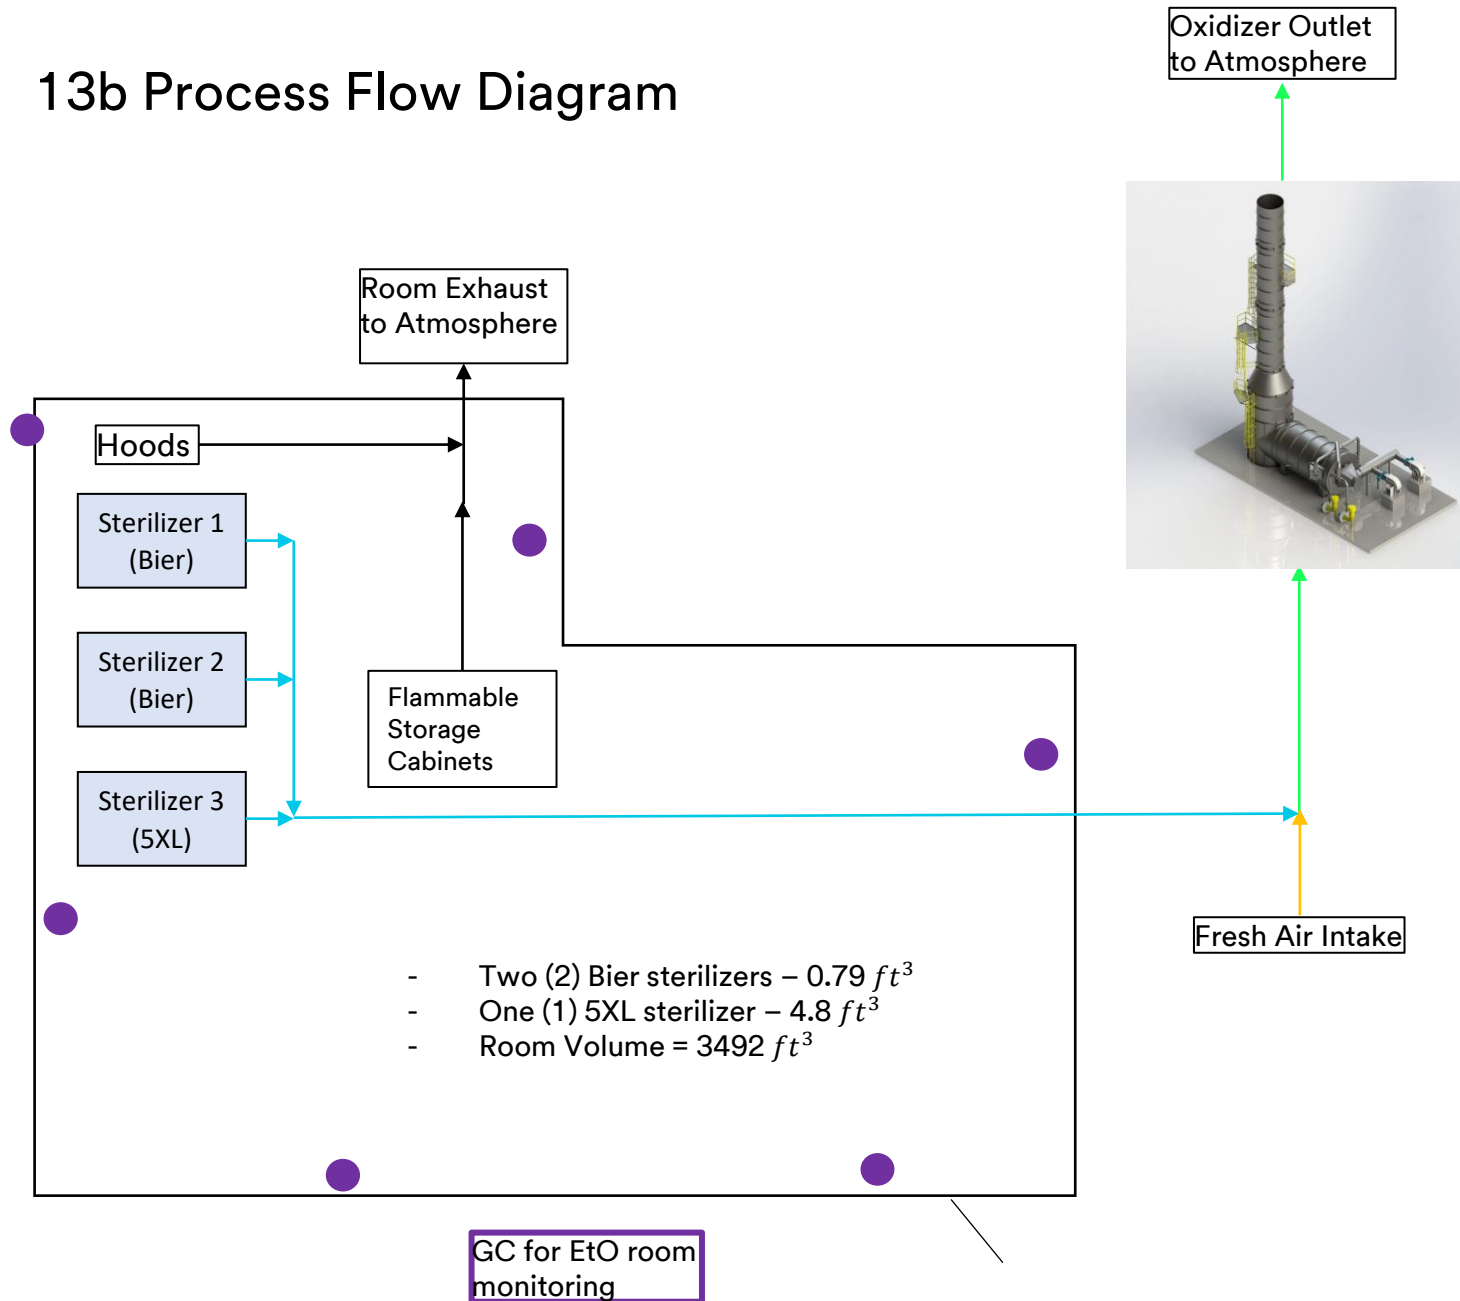

- Sterilizer EtO Exhaust
- Combined Airflow
- Fresh Air Intake
- GC for EtO room monitoring



- This is a QA/QC test of a medical product.
- Sample batch test
- Product is to industry standard to show sterilization